

RESL CUSTOMER EXPORT CONTROL AGREEMENT

It is the Radiological and Environmental Sciences Laboratory's (RESL) policy to conduct business in accordance with all applicable U.S. export control laws and regulations. It is also RESL's policy that its Customers comply with U.S. export control laws and regulations. Therefore, Customer agrees to the following:

1. Because products, technical data, and technical assistance (i.e., services) provided to Customer by RESL may be subject to U.S. export control laws and regulations, (i) transactions with certain persons and companies and (ii) the export or reexport of certain types and levels of products, technical data, and services are prohibited or restricted.
2. Customer acknowledges that it is responsible for its own compliance with U.S. export control laws and regulations. Customer further agrees that it assumes the responsibility to obtain all necessary U.S. export licenses or other U.S. governmental authorizations, as well as all liability for the failure to do so.
3. Customer acknowledges that export control requirements may change and that the export or reexport of RESL products, technical data, and services without an export license or other appropriate governmental authorization may result in criminal and/or civil liability.
4. The obligations and requirements described herein shall survive the expiration or termination of any agreement or contract between RESL and Customer.

GrF31 Participating Laboratories

Lab Code	Lab Name	Matrix Code
ADEM01	Alabama Department of Environmental Management	GrF
ADFC99	Abu Dhabi Quality and Conformity Council-Central Testing Lab	GrF
AFOH01	USAFSAM/OEA	GrF
ANTE01	ALS Environmental - Fort Collins, CO	GrF
ARGO01	Idaho National Laboratory	GrF
ARPL01	Analytical Support Operations - Radiochemical Processing Lab	GrF
ARSL01	ARS International, LLC	GrF
ASUK99	NAS Radiochemistry Group	GrF
AY1201	Consolidated Nuclear Security, LLC, Analytical Chemistry Organization Laboratory	GrF
CDHS01	California Department of Public Health	GrF
CESL01	Lawrence Livermore National Laboratory - EMRL	GrF
CHMH01	222-S Laboratory	GrF
CMRC01	Carlsbad Environmental Monitoring and Research Center	GrF
DEHS01	Department of Environmental Health & Safety	GrF
DINL99	Departamento Ingeniería Nuclear y Mecánica de Fluidos	GrF
DPHE01	Colorado Dept. of Public Health & Env. / Laboratory Services Div.	GrF
DRMG01	CNS Pantex - D&RMG	GrF
ELCS01	Energy Labs - College Station	GrF
ELIW01	Energy Laboratories, Inc.	GrF
EPAL01	U.S. EPA ORIA/NCRFO	GrF
ERCL01	Washington State Public Health Laboratories	GrF
EULC01	EnergySolutions, LLC	GrF
FDHE01	Florida Dept of Health Environmental Laboratory	GrF
FDOH01	Florida Dept. of Health, Mobile Environmental Radiological Lab	GrF
FMEC99	Foods and Water Laboratories Center	GrF
GENE01	GEL Laboratories, LLC	GrF
HCAL01	Hazards Control Analytical Lab	GrF
HECR01	SC Dept. Health and Environmental Control Radiological Laboratory	GrF
HERR01	Washington Closure Hanford	GrF
ISUP01	ISU - Department of Physics/Health Physics/EAL	GrF
JAEC99	Research Laboratories and Information Directorate	GrF
KDHE01	Kansas Dept. of Health & Environment	GrF
KSCF01	Kennedy Space Center, HP Laboratory	GrF
LAEC99	Lebanese Atomic Energy Commission - Environmental Radiation	GrF
LDRA99	Laboratori de Radiologia Ambiental-Universitat de Barcelona	GrF
LGCL99	LGC Ltd	GrF
LOCK03	Advanced Test Reactor (ATR) Complex Radioanalytical Laboratory	GrF
MAHP59	Materials Assessment and Health Physics Group	GrF
MALA99	Asia Lab (M) Sdn. Bhd.	GrF
MART03	Radioactive Material Analysis Laboratory	GrF
MDPH01	MDPH-Radiation Control Program	GrF
NARL01	National Air and Radiation Environmental Laboratory	GrF
NARL02	USEPA - NAREL - MERL	GrF
NCNS99	Radioanalytical Laboratory	GrF
NESI01	B&W Technical Services-Radioisotope & Analytical Chemistry Laboratory	GrF
NJDH01	New Jersey Dept. of Health, PHEL, ECLS	GrF
NOCS99	National Oceanography Centre, Southampton	GrF
ODHL01	Ohio Department of Health Laboratory	GrF
ORIS01	ORISE/IEAV	GrF
OTLI01	Outreach Technologies, Inc.	GrF
QUAN01	TestAmerica St. Louis	GrF
QUAN03	TestAmerica Laboratories - Richland	GrF
RAVR99	Radiactividad Ambiental y Vigilancia Radiologica	GrF
RPSC01	Radiation Protection Service	GrF
SANC99	RadioAnalysis, South Africa Nuclear Energy Corp.	GrF
SEML01	SRS Environmental Monitoring Laboratory	GrF

SOUT01	Southwest Research Institute	GrF
SRPD01	Sandia National Laboratories, Radiation Protection Sample Diagnostics	GrF
TDHL01	Texas Department of State Health Services Laboratory	GrF
TELE01	TELEDYNE BROWN ENGINEERING - ENVIRONMENTAL SERVICES	GrF
TELE02	ATI Environmental, Inc., Midwest Lab	GrF
TMAO01	EBERLINE SERVICES OAK RIDGE LABORATORY	GrF
TNUT01	St. Louis USACE FUSRAP Laboratory	GrF
UPVL99	Lab Radiactividad Ambiental. Univ. Politecnica Valencia	GrF
URSL01	UNLV Radioanalytical Services Laboratory	GrF
USED99	National Center for Nuclear Energy, Sciences and Techniques	GrF
WEST04	PACE ANALYTICAL SERVICES, PITTSBURGH	GrF
WIPP01	WIPP Laboratories	GrF
WSHL01	Wisconsin State Laboratory of Hygiene	GrF
WVDP01	WVDP Environmental Laboratory	GrF
WVPL01	WVDP Radiation Protection Lab	GrF

Laboratories Not Reporting GrF31

Lab Code	Lab Name	Matrix Code
CEEA99	Laboratorio de Vigilancia Ambiental Radiactiva	GrF
GPCL01	Georgia Power Company Environmental Laboratory	GrF
MART02	United States Enrichment Corporation	GrF
RMCL99	Royal Scientific Society - Radiation Protection Lab	GrF

Study Reference Values

MAPEP-14-GrF31

Radiological Reference Date: 08/01/2014

Analyte	Ref Value	Ref Unc
Radiological		Units: (Bq/sample)
Gross alpha	0.53	0.02
Gross beta	1.06	0.04

Sample Statistical Summary

MAPEP-14-GrF31

Radiological Reference Date: 08/01/2014

Analyte	T(1)	A(2)	Grand(3) Mean	Std Dev	Ref Value	Ref Unc	Acceptance Range
Radiological						Units: (Bq/sample)	
Gross alpha	71	48	0.36	0.15	0.53	0.02	0.16 - 0.90
Gross beta	71	67	1.04	0.11	1.06	0.04	0.53 - 1.59

- Note:** (1) T = Total number of laboratories reporting analyte.
 (2) A = Number of laboratories with 'Acceptable' performance.
 (3) Mean excludes values derived as total metals and values indicated as "Not Acceptable".

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP $<$ 2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15% $<$ RP \leq 30%
- 4) NOT ACCEPTABLE.....RP $>$ 30%

RP = Relative Precision

Flag Summary Report

MAPEP-14-GrF31

Radiological

<u>Analyte</u>	<u>A</u>	<u>W</u>	<u>RW</u>	<u>N</u>
Gross alpha	48			23
Gross beta	67			4



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ADEM01) Alabama Department of Environmental Management
 Montgomery Laboratory
 Montgomery, AL 36110

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.041	0.53	N		-92.3	0.16 - 0.90	0.001	A
Gross beta	0.010	1.06	N		-99.1	0.53 - 1.59	0.001	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ADFC99) Abu Dhabi Quality and Conformity Council-Central Testing Lab
 Radiation Lab
 Abu Dhabi, - -

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.32	0.53	A		-39.6	0.16 - 0.90	0.05	W
Gross beta	0.89	1.06	A		-16.0	0.53 - 1.59	0.05	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (AFOH01) USAFSAM/OEA
 2510 Fifth Street, Area B
 Wright-Patterson AFB, OH 45433-7913

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.413	0.53	A		-22.1	0.16 - 0.90	0.081	W
Gross beta	1.049	1.06	A		-1.0	0.53 - 1.59	0.066	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ANTE01) ALS Environmental - Fort Collins, CO
 225 Commerce Drive
 Fort Collins, CO 80524-1416

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.447	0.53	A		-15.7	0.16 - 0.90	0.040	A
Gross beta	1.03	1.06	A		-2.8	0.53 - 1.59	0.08	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ARGO01) Idaho National Laboratory
 INL, Materials and Fuels Complex
 Idaho Falls, ID 83415

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	4.76E-01	0.53	A		-10.2	0.16 - 0.90	3.56E-02	A
Gross beta	1.03E+00	1.06	A		-2.8	0.53 - 1.59	7.31E-02	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(ARPL01) Analytical Support Operations - Radiochemical Processing Lab

PO Box 999

Richland, WA 99354

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.157	0.53	N		-70.4	0.16 - 0.90	0.009	A
Gross beta	0.96	1.06	A		-9.4	0.53 - 1.59	0.03	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(ARSL01) ARS International, LLC

2609 North River Road

Port Allen, LA 70767

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.153	0.53	N		-71.1	0.16 - 0.90	0.021	A
Gross beta	1.038	1.06	A		-2.1	0.53 - 1.59	0.128	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ASUK99) NAS Radiochemistry Group
 A38.1 AWE,
 Reading, Berkshire RG7 4PR

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.552	0.53	A		4.2	0.16 - 0.90	0.027	A
Gross beta	1.288	1.06	A		21.5	0.53 - 1.59	0.018	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(AY1201) Consolidated Nuclear Security, LLC, Analytical Chemistry Organization Laboratory
 Y12, NSC, Bldg. 9995, Rm 142
 Oak Ridge, TN 37831-8189

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.641	0.53	A		20.9	0.16 - 0.90	0.068	A
Gross beta	1.11	1.06	A		4.7	0.53 - 1.59	0.079	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (CDHS01) California Department of Public Health
 Drinking Water & Radiation Lab.
 Richmond, CA 94804-6403

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.166	0.53	A		-68.7	0.16 - 0.90	0.0105	A
Gross beta	1.10	1.06	A		3.8	0.53 - 1.59	0.0153	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (CESL01) Lawrence Livermore National Laboratory - EMRL
 7000 East Avenue
 Livermore, CA 94551

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.19E-01	0.53	N		-77.5	0.16 - 0.90	1.35E-02	A
Gross beta	1.10E+00	1.06	A		3.8	0.53 - 1.59	3.33E-02	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(CHMH01) 222-S Laboratory

P.O. Box 250, MS T6-10

Richland, WA 99352

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.244	0.53	A		-54.0	0.16 - 0.90	0.0542	W
Gross beta	0.893	1.06	A		-15.8	0.53 - 1.59	0.0608	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (CMRC01) Carlsbad Environmental Monitoring and Research Center
 1400 University Dr.
 Carlsbad, NM 88220

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.106	0.53	N		-80.0	0.16 - 0.90	0.003	A
Gross beta	1.094	1.06	A		3.2	0.53 - 1.59	0.016	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (DEHS01) Department of Environmental Health & Safety
 North Carolina State Univ.
 Raleigh, NC 27695-8007

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.37	0.53	A		-30.2	0.16 - 0.90	0.02	A
Gross beta	0.95	1.06	A		-10.4	0.53 - 1.59	0.04	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2%<=RP<=15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP<=30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (DINL99) Departamento Ingeniería Nuclear y Mecánica de Fluidos
 Alameda de Urquijo s/n
 Bilbao, Vizcaya 48013

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.177	0.53	A		-66.6	0.16 - 0.90	0.008	A
Gross beta	1.04	1.06	A		-1.9	0.53 - 1.59	0.027	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(DPHE01) Colorado Dept. of Public Health & Env. / Laboratory Services Div.

8100 Lowry Blvd
Denver, CO 80230

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.20	0.53	A		-62.3	0.16 - 0.90	0.03	A
Gross beta	1.0	1.06	A		-5.7	0.53 - 1.59	0.03	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(DRMG01) CNS Pantex - D&RMG

Bldg 12-122

Amarillo, TX 79120-0020

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	3.35E-01	0.53	A		-36.8	0.16 - 0.90	2.83E-02	A
Gross beta	1.08E+00	1.06	A		1.9	0.53 - 1.59	2.59E-02	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ELCS01) Energy Labs - College Station
 415 Graham RD
 College Station, Tx 77845

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.33	0.53	A		-37.7	0.16 - 0.90	0.01	A
Gross beta	0.98	1.06	A		-7.5	0.53 - 1.59	0.03	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(ELIW01) Energy Laboratories, Inc.

2393 Salt Creek HWY

Casper, Wy 82601

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.41	0.53	A		-22.6	0.16 - 0.90	0.035	A
Gross beta	0.95	1.06	A		-10.4	0.53 - 1.59	0.026	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(EPAL01) U.S. EPA ORIA/NCRFO

4220 S. Maryland Parkway

Las Vegas, NV 89119-6721

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.137	0.53	N		-74.2	0.16 - 0.90	.008	A
Gross beta	1.024	1.06	A		-3.4	0.53 - 1.59	.038	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ERCL01) Washington State Public Health Laboratories
 1610 N.E. 150th Street
 Shoreline, WA 98155-9701

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.099	0.53	N		-81.3	0.16 - 0.90	0.012	A
Gross beta	0.981	1.06	A		-7.5	0.53 - 1.59	0.025	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(EULC01) EnergySolutions, LLC

I-80, Exit 46

Clive, UT 84029

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	.1177	0.53	N		-77.8	0.16 - 0.90	.026	W
Gross beta	1.1036	1.06	A		4.1	0.53 - 1.59	.262	W

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (FDHE01) Florida Dept of Health Environmental Laboratory
 PO Box 680069
 Orlando, FL 32868-0069

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.427	0.53	A		-19.4	0.16 - 0.90	0.027	A
Gross beta	1.073	1.06	A		1.2	0.53 - 1.59	0.008	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(FDOH01) Florida Dept. of Health, Mobile Environmental Radiological Lab
 PO Box 680069
 Orlando, FL 32868-0069

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.49	0.53	A		-7.5	0.16 - 0.90	.02	A
Gross beta	.96	1.06	A		-9.4	0.53 - 1.59	.01	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (FMEC99) Foods and Water Laboratories Center
 Ministry of Regional Municipalities and Water Resources
 Muscat, seeb 111

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.374	0.53	A		-29.4	0.16 - 0.90	0.05	A
Gross beta	0.892	1.06	A		-15.8	0.53 - 1.59	0.06	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(GENE01) GEL Laboratories, LLC

2040 Savage Road

Charleston, SC 29407

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.433	0.53	A		-18.3	0.16 - 0.90	0.0791	W
Gross beta	1.06	1.06	A		0.0	0.53 - 1.59	0.0474	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (HCAL01) Hazards Control Analytical Lab
 Lawrence Livermore National
 Livermore, CA 94551

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	.134	0.53	N		-74.7	0.16 - 0.90	.031	W
Gross beta	1.23	1.06	A		16.0	0.53 - 1.59	.13	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(HECR01) SC Dept. Health and Environmental Control Radiological Laboratory
 8231 Parklane Road
 Columbia, SC 29223

Radiological					Units: (Bq/sample)			
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.0768	0.53	N		-85.5	0.16 - 0.90	0.0255	N
Gross beta	0.0642	1.06	N		-93.9	0.53 - 1.59	0.0240	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP $< 2\%$
- 2) ACCEPTABLE..... $2\% \leq RP \leq 15\%$
- 3) ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$
- 4) NOT ACCEPTABLE.....RP $> 30\%$

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (HERR01) Washington Closure Hanford
 Radiological Counting Facility
 Richland, WA 99352

Radiological					Units: (Bq/sample)			
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.13	0.53	N		-75.5	0.16 - 0.90	0.04	N
Gross beta	1.62	1.06	N		52.8	0.53 - 1.59	0.13	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2%<=RP<=15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP<=30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ISUP01) ISU - Department of Physics/Health Physics/EAL
 785 S. 8th Ave, Rm 120
 Pocatello, ID 83209-8106

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.332	0.53	A		-37.4	0.16 - 0.90	0.018	A
Gross beta	0.890	1.06	A		-16.0	0.53 - 1.59	0.015	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (JAEC99) Research Laboratories and Information Directorate
 Jordan Atomic Energy Commission
 Amman, Jordan 70 (11934)

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.155	0.53	N		-70.8	0.16 - 0.90	0.014	A
Gross beta	1.170	1.06	A		10.4	0.53 - 1.59	0.048	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (KDHE01) Kansas Dept. of Health & Environment
 6810 SE Dwight Street
 Topeka, KS 66620

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.26	0.53	A		-50.9	0.16 - 0.90	0.03	A
Gross beta	1.03	1.06	A		-2.8	0.53 - 1.59	0.03	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (KSCF01) Kennedy Space Center, HP Laboratory
 IHA-023
 Kennedy Space Center, FL 32899

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.15	0.53	N		-71.7	0.16 - 0.90	0.0062	A
Gross beta	0.5983	1.06	A		-43.6	0.53 - 1.59	0.0200	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (LAEC99) Lebanese Atomic Energy Commission - Environmental Radiation
 National Council for Scientific Research
 Beirut, Beirut 1107 2260

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.34	0.53	A		-35.8	0.16 - 0.90	0.004	N
Gross beta	1.09	1.06	A		2.8	0.53 - 1.59	0.02	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(LDRA99) Laboratori de Radiologia Ambiental-Universitat de Barcelona

Facultat de Quimica

Barcelona, Catalunya 08028

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.41	0.53	A		-22.6	0.16 - 0.90	0.04	A
Gross beta	1.02	1.06	A		-3.8	0.53 - 1.59	0.17	W

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(LGCL99) LGC Ltd

Queens Road

Teddington, Middlesex TW11 0LY

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.508	0.53	A		-4.2	0.16 - 0.90	0.073	A
Gross beta	1.097	1.06	A		3.5	0.53 - 1.59	0.088	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (LOCK03) Advanced Test Reactor (ATR) Complex Radioanalytical Laboratory
 INL/Battelle Energy Alliance, LLC
 Idaho Falls, ID 83415-7111

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.16	0.53	A		-69.8	0.16 - 0.90	0.02	A
Gross beta	1.24	1.06	A		17.0	0.53 - 1.59	0.10	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (MAHP59) Materials Assessment and Health Physics Group
 Imperial College Reactor Centre
 Ascot, Berkshire SL5 7TE

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.56	0.53	A		5.7	0.16 - 0.90	0.06	A
Gross beta	1.02	1.06	A		-3.8	0.53 - 1.59	0.06	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(MALA99) Asia Lab (M) Sdn. Bhd.

No. 14, JLN USJ 1/1

Subang Jaya, Selangor 47600

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.33	0.53	A		-37.7	0.16 - 0.90	0.03	A
Gross beta	1.09	1.06	A		2.8	0.53 - 1.59	0.04	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (MART03) Radioactive Material Analysis Laboratory
 ORNL
 Oak Ridge, TN 37831-6223

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.218	0.53	A		-58.9	0.16 - 0.90	0.023	A
Gross beta	1.16	1.06	A		9.4	0.53 - 1.59	0.05	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (MDPH01) MDPH-Radiation Control Program
 MERL-Room 002
 Jamaica Plain, MA 02130-3597

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.13	0.53	N		-75.5	0.16 - 0.90	0.01	A
Gross beta	1.03	1.06	A		-2.8	0.53 - 1.59	0.02	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (NARL01) National Air and Radiation Environmental Laboratory
 540 S. Morris Ave.
 Montgomery, AL 36115-2601

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.116	0.53	N		-78.1	0.16 - 0.90	0.0162	A
Gross beta	1.02	1.06	A		-3.8	0.53 - 1.59	0.0551	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(NARL02) USEPA - NAREL - MERL

540 S Morris Ave

Montgomery, AL 36115

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.159	0.53	A		-70.0	0.16 - 0.90	0.00888	A
Gross beta	1.05	1.06	A		-0.9	0.53 - 1.59	0.0189	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (NCNS99) Radioanalytical Laboratory
 National Center for Nuclear Sciences and Technologies
 Thabet Ariana, Ariana 2020

Radiological					Units: (Bq/sample)			
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.0142	0.53	N		-97.3	0.16 - 0.90	0.0039	W
Gross beta	0.0684	1.06	N		-93.5	0.53 - 1.59	0.0139	W

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(NESI01) B&W Technical Services-Radioisotope & Analytical Chemistry Laboratory
 Lynchburg Technology Center
 Lynchburg, VA 24504-5447

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.358	0.53	A		-32.5	0.16 - 0.90	0.026	A
Gross beta	1.06	1.06	A		0.0	0.53 - 1.59	0.03	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (NJDH01) New Jersey Dept. of Health, PHEL, ECLS
 3 Schwarzkopf Drive
 West Trenton, NJ 08628

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.5846	0.53	A		10.3	0.16 - 0.90	0.0047	N
Gross beta	1.143	1.06	A		7.8	0.53 - 1.59	0.011	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (NOCS99) National Oceanography Centre, Southampton
 GAU-Radioanalytical
 Southampton, Hampshire SO14 3ZH

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.28	0.53	A		-47.2	0.16 - 0.90	0.02	A
Gross beta	1.22	1.06	A		15.1	0.53 - 1.59	0.02	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (ODHL01) Ohio Department of Health Laboratory
 8995 E Main Street
 Reynoldsburg, OH 43068

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.154	0.53	N		-70.9	0.16 - 0.90	0.011	A
Gross beta	1.110	1.06	A		4.7	0.53 - 1.59	0.019	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(ORIS01) ORISE/IEAV

PO Box 117

Oak Ridge, TN 37831-0117

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.314	0.53	A		-40.8	0.16 - 0.90	0.014	A
Gross beta	1.058	1.06	A		-0.2	0.53 - 1.59	0.015	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(OTLI01) Outreach Technologies, Inc.

311 N. Aspen

Broken Arrow, OK 74012-

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	.196	0.53	A		-63.0	0.16 - 0.90	.001	N
Gross beta	1.14	1.06	A		7.5	0.53 - 1.59	.020	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(QUAN01) TestAmerica St. Louis
 13715 Rider Trail North
 Earth City, MO 63045-1205

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.0687	0.53	N		-87.0	0.16 - 0.90	0.00469	A
Gross beta	0.864	1.06	A		-18.5	0.53 - 1.59	0.0438	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (QUAN03) TestAmerica Laboratories - Richland
 2800 GEORGE WASHINGTON WAY
 RICHLAND, WA 99354-

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.181	0.53	A		-65.8	0.16 - 0.90	0.0200	A
Gross beta	1.18	1.06	A		11.3	0.53 - 1.59	0.0913	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (RAVR99) Radiactividad Ambiental y Vigilancia Radiologica
 CIEMAT (Ed 70 P2 D11)
 Madrid, Madrid 28040

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.81	0.53	A		52.8	0.16 - 0.90	0.0085	N
Gross beta	1.003	1.06	A		-5.4	0.53 - 1.59	0.027	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(RPSC01) Radiation Protection Service

Ontario Ministry of Labour

Weston, Ontario M9P 3T1

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.12	0.53	N		-77.4	0.16 - 0.90	0.02	W
Gross beta	1.29	1.06	A		21.7	0.53 - 1.59	0.13	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (SANC99) RadioAnalysis, South Africa Nuclear Energy Corp.
 Sample Receipt Gate 1
 Pretoria, Gauteng 0001

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.173	0.53	A		-67.4	0.16 - 0.90	0.014	A
Gross beta	1.03	1.06	A		-2.8	0.53 - 1.59	0.03	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (SEML01) SRS Environmental Monitoring Laboratory
 Bldg 735-B
 Aiken, SC 29808

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.298	0.53	A		-43.8	0.16 - 0.90	0.074	W
Gross beta	1.08	1.06	A		1.9	0.53 - 1.59	0.22	W

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (SOUT01) Southwest Research Institute
 6220 Culebra Rd.
 San Antonio, TX 78228-0510

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.489	0.53	A		-7.7	0.16 - 0.90	0.0337	A
Gross beta	1.02	1.06	A		-3.8	0.53 - 1.59	0.0615	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(SRPD01) Sandia National Laboratories, Radiation Protection Sample Diagnostics
 PO Box 5800, MS1103
 Albuquerque, NM 87185-1103

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.675	0.53	A		27.4	0.16 - 0.90	0.013	N
Gross beta	0.995	1.06	A		-6.1	0.53 - 1.59	0.034	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (TDHL01) Texas Department of State Health Services Laboratory
 1100 W 49th Street
 Austin, TX 78756

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.299	0.53	A		-43.6	0.16 - 0.90	0.015	A
Gross beta	1.013	1.06	A		-4.4	0.53 - 1.59	0.021	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(TELE01) TELEDYNE BROWN ENGINEERING - ENVIRONMENTAL SERVICES

2508 Quality Lane

Knoxville, TN 37931-6819

Radiological							Units: (Bq/sample)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.153	0.53	N		-71.1	0.16 - 0.90	0.033	W
Gross beta	0.977	1.06	A		-7.8	0.53 - 1.59	0.060	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (TELE02) ATI Environmental, Inc., Midwest Lab
 700 Landwehr Road
 Northbrook, IL 60062-

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.167	0.53	A		-68.5	0.16 - 0.90	0.03	W
Gross beta	1.214	1.06	A		14.5	0.53 - 1.59	0.07	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (TMAO01) EBERLINE SERVICES OAK RIDGE LABORATORY
 601 SCARBORO RD
 OAK RIDGE, TN 37830-

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.158	0.53	N		-70.2	0.16 - 0.90	0.012	A
Gross beta	1.081	1.06	A		2.0	0.53 - 1.59	0.026	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (TNUT01) St. Louis USACE FUSRAP Laboratory
 8945 LATTY AVE
 BERKELEY, MO 63134-

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	.6051	0.53	A		14.2	0.16 - 0.90	.0186	A
Gross beta	.9970	1.06	A		-5.9	0.53 - 1.59	.0281	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (UPVL99) Lab Radiactividad Ambiental. Univ. Politecnica Valencia
 CAMINO DE VERA, 14
 VALENCIA, VALENCIA 46022

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.277	0.53	A		-47.7	0.16 - 0.90	0.003	N
Gross beta	1.03	1.06	A		-2.8	0.53 - 1.59	0.01	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (URSL01) UNLV Radioanalytical Services Laboratory
 Campus Mail Stop 453037
 Las Vegas, NV 89154-3037

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.223	0.53	A		-57.9	0.16 - 0.90	0.0137	A
Gross beta	0.880	1.06	A		-17.0	0.53 - 1.59	0.0278	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(USED99) National Center for Nuclear Energy, Sciences and Techniques
 CNESTEN BP 1382

RABAT, RABAT RP 10001

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1	0.53	N		88.7	0.16 - 0.90	1	N
Gross beta	1	1.06	A		-5.7	0.53 - 1.59	1	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (WEST04) PACE ANALYTICAL SERVICES, PITTSBURGH
 1638 Roseytown Road
 Greensburg, PA 15601

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.388	0.53	A		-26.8	0.16 - 0.90	.0729	W
Gross beta	.925	1.06	A		-12.7	0.53 - 1.59	.168	W

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31

(WIPP01) WIPP Laboratories

1400 University Drive

Carlsbad, NM 88220

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	4.02E-01	0.53	A		-24.2	0.16 - 0.90	2.55E-02	A
Gross beta	1.18E+00	1.06	A		11.3	0.53 - 1.59	2.17E-02	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (WSHL01) Wisconsin State Laboratory of Hygiene
 2601 Agriculture Drive
 Madison, WI 53718

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.3859	0.53	A		-27.2	0.16 - 0.90	0.0222	A
Gross beta	0.9125	1.06	A		-13.9	0.53 - 1.59	0.0139	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (WVDP01) WVDP Environmental Laboratory
 10282 Rock Springs Road
 West Valley, NY 14171

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.194	0.53	A		-63.4	0.16 - 0.90	0.0116	A
Gross beta	1.03	1.06	A		-2.8	0.53 - 1.59	0.0133	N

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-14-GrF31
 (WVPL01) WVDP Radiation Protection Lab
 10282 Rock Springs Rd
 West Valley, NY 14171

Radiological						Units: (Bq/sample)		
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.0902	0.53	N		-83.0	0.16 - 0.90	0.0105	A
Gross beta	1.0286	1.06	A		-3.0	0.53 - 1.59	0.0273	A

Radiological Reference Date: August 1, 2014

Gross Alpha Flags:

A = Result acceptable, Bias \leq +/- 70% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 70% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias \leq +/- 50% with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $>$ +/- 50% or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).


Uncertainty Flags:

- 1) NOT ACCEPTABLE.....RP<2%
- 2) ACCEPTABLE.....2% \leq RP \leq 15%
- 3) ACCEPTABLE WITH WARNING.....15%<RP \leq 30%
- 4) NOT ACCEPTABLE.....RP>30%

RP = Relative Precision

Gross alpha


MAPEP-14-GrF31

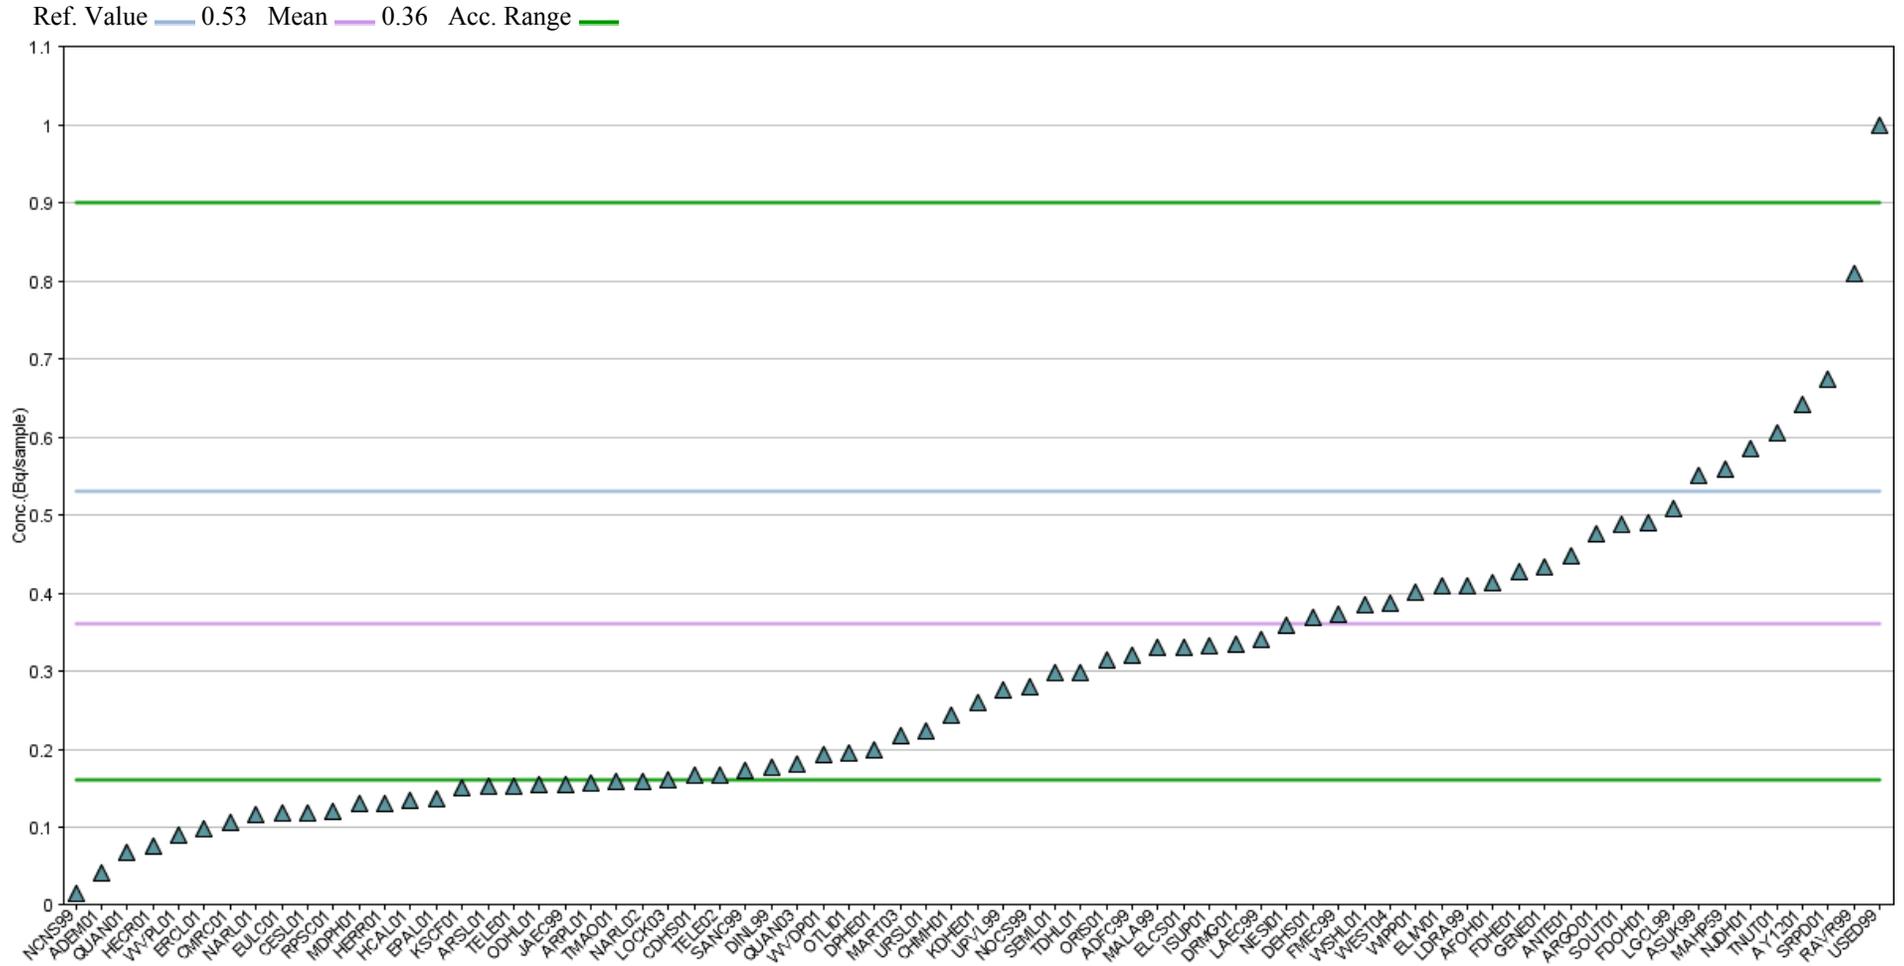

Note: This chart shows only data points with values between -0.40 and 1.12 (± 5 Standard Deviations)


Gross beta

MAPEP-14-GrF31

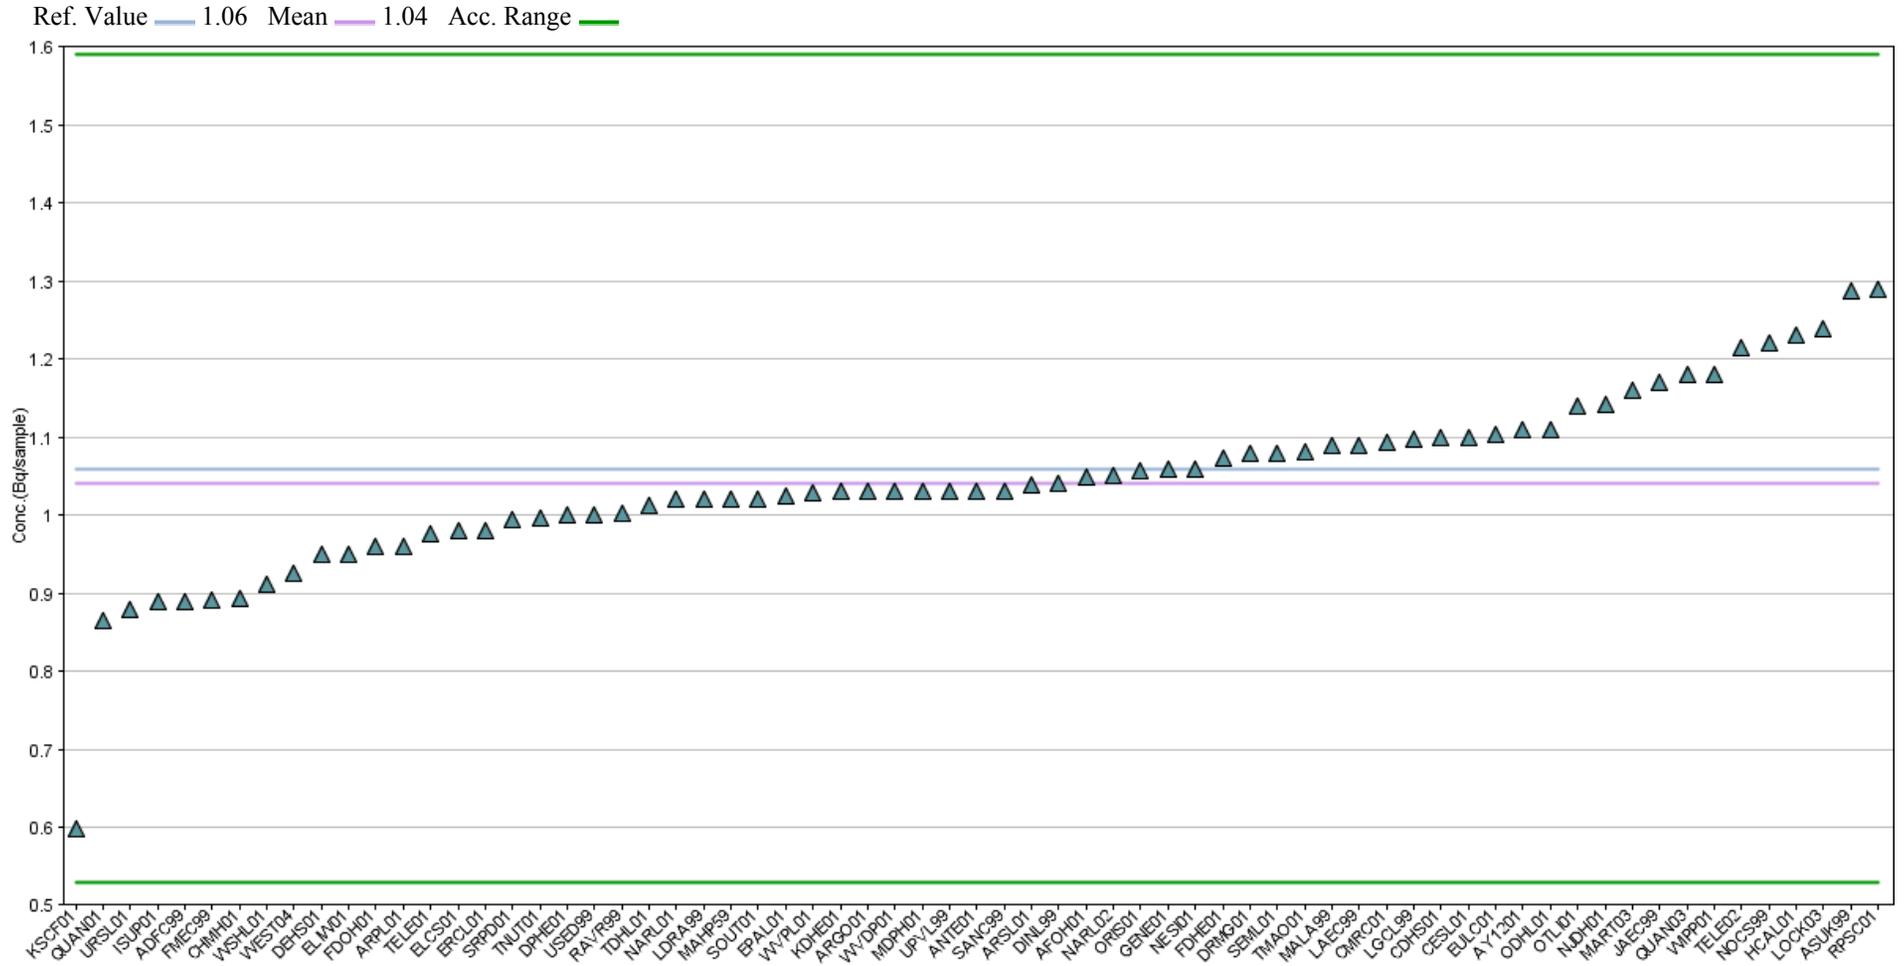


Note: This chart shows only data points with values between 0.49 and 1.60 (± 5 Standard Deviations)

The intent of the distribution graphs contained within this report is to graphically demonstrate to users how % Bias data within the current MAPEP Series appears when examined by matrix, by analyte, by method of sample preparation or by method of detection. The data points (small 'dots') plot the bias (or z-score for organic constituents) of each of the analytes in each of the matrices. The BLACK small vertical line inside the small rectangle at the top of the data distribution graph is the mean of the population of the bias shown for that analyte in the matrix.

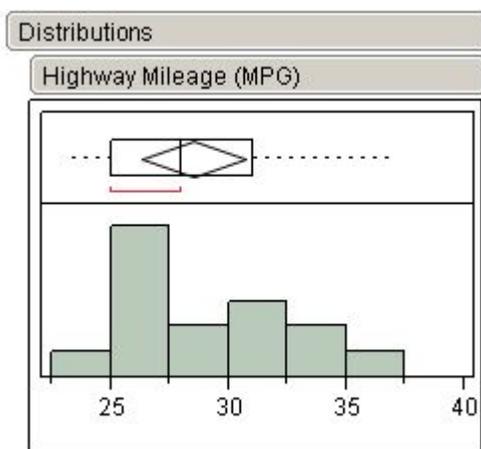

Moments	
Mean	28.466667
Std Dev	3.9797104
Std Err Mean	1.0275568
Upper 95% Mean	30.670557
Lower 95% Mean	26.262776
N	15
Sum Wgt	15
Sum	427
Variance	15.838095
Skewness	0.7309964
Kurtosis	-0.165153
CV	13.980247
N Missing	0

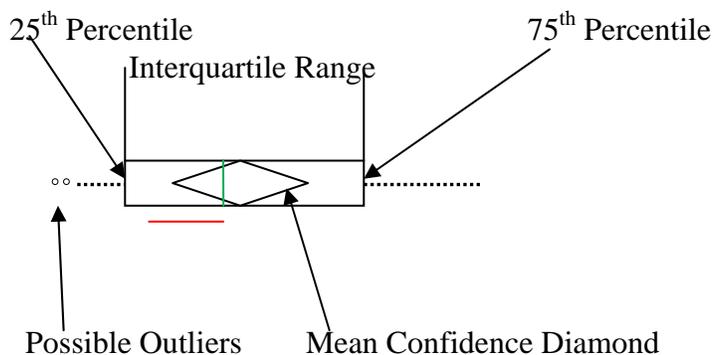


The box plots summarize the distribution of points for each analyte. The ends of the box are the 25th and 75th quantiles. The difference between the quartiles is the interquartile range. The line across the middle of the box identifies the median bias value. Each box has lines, sometimes called whiskers, which extend from each end. The whiskers extend from the ends of the small box to the outermost data point that falls within the distances computed. Any potential outliers are represented as small black dots.

The box plot of the bias data points and the mean visually illustrate the breadth of the distribution and where any potential outliers in the distribution might lie. The moments for the distribution plot are provided below the Bias plot. In some cases, N becomes very small and thus developed statistics may not accurately reflect estimates of the population if N were a significantly larger value.

GrF Distribution by Detection Method

Distributions Analyte_Detection=Gross alpha
Beta Counting - 2 pi gas flow proportional counter

Bias

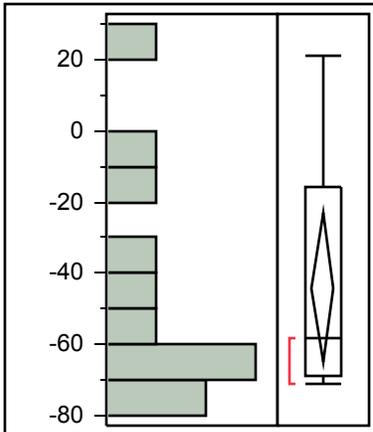

Quantiles

100.0%	maximum	20.9
99.5%		20.9
97.5%		20.9
90.0%		15.18
75.0%	quartile	-15.7
50.0%	median	-57.9
25.0%	quartile	-68.7
10.0%		-71.1
2.5%		-71.1
0.5%		-71.1
0.0%	minimum	-71.1


Summary Statistics

Mean	-44.00909
Std Dev	31.013399
Std Err Mean	9.3508916
Upper 95% Mean	-23.17401
Lower 95% Mean	-64.84418
N	11

GrF Distribution by Detection Method

Distributions Analyte_Detection=Gross alpha
Beta Counting - liquid scintillation counter

Bias

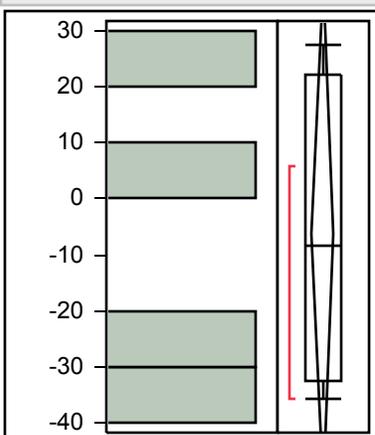

Quantiles

100.0%	maximum	27.4
99.5%		27.4
97.5%		27.4
90.0%		27.4
75.0%	quartile	21.975
50.0%	median	-8.45
25.0%	quartile	-32.5
10.0%		-35.8
2.5%		-35.8
0.5%		-35.8
0.0%	minimum	-35.8


Summary Statistics

Mean	-6.325
Std Dev	28.376208
Std Err Mean	14.188104
Upper 95% Mean	38.827879
Lower 95% Mean	-51.47788
N	4

GrF Distribution by Detection Method

Distributions Analyte_Detection=Gross alpha Gross
Alpha/Beta - 2 pi gas flow proportional counter

Bias

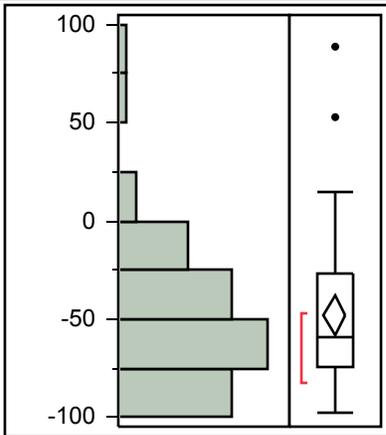

Quantiles

100.0%	maximum	88.7
99.5%		88.7
97.5%		74.34
90.0%		-6.18
75.0%	quartile	-27.2
50.0%	median	-58.9
25.0%	quartile	-74.7
10.0%		-81.98
2.5%		-95.3
0.5%		-97.3
0.0%	minimum	-97.3

Summary Statistics


Mean	-48.10727
Std Dev	35.63921
Std Err Mean	4.8055901
Upper 95% Mean	-38.47264
Lower 95% Mean	-57.7419
N	55

GrF Distribution by Detection Method

Distributions

Analyte_Detection=Gross alpha Other

Bias

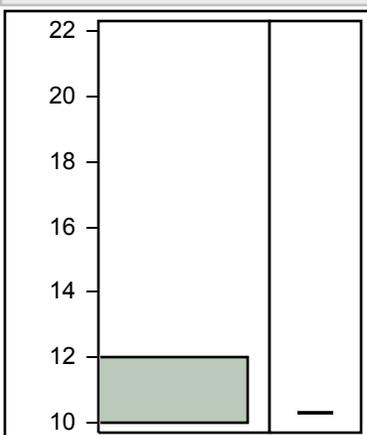

Quantiles

100.0%	maximum	10.3
99.5%		10.3
97.5%		10.3
90.0%		10.3
75.0%	quartile	10.3
50.0%	median	10.3
25.0%	quartile	10.3
10.0%		10.3
2.5%		10.3
0.5%		10.3
0.0%	minimum	10.3


Summary Statistics

Mean	10.3
Std Dev	.
Std Err Mean	.
Upper 95% Mean	.
Lower 95% Mean	.
N	1

GrF Distribution by Detection Method

Distributions Analyte_Detection=Gross beta Beta
Counting - 2 pi gas flow proportional counter

Bias

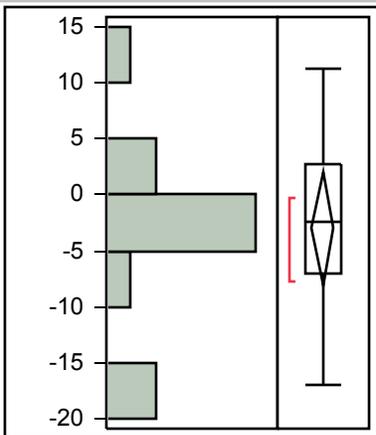

Quantiles

100.0%	maximum	11.3
99.5%		11.3
97.5%		11.3
90.0%		9.32
75.0%	quartile	2.8
50.0%	median	-2.45
25.0%	quartile	-6.95
10.0%		-16.7
2.5%		-17
0.5%		-17
0.0%	minimum	-17


Summary Statistics

Mean	-3.016667
Std Dev	8.0371674
Std Err Mean	2.3201304
Upper 95% Mean	2.0899059
Lower 95% Mean	-8.123239
N	12

GrF Distribution by Detection Method

Distributions Analyte_Detection=Gross beta
Beta Counting - liquid scintillation counter

Bias

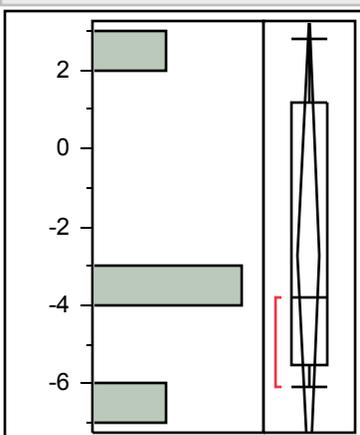

Quantiles

100.0%	maximum	2.8
99.5%		2.8
97.5%		2.8
90.0%		2.8
75.0%	quartile	1.15
50.0%	median	-3.8
25.0%	quartile	-5.525
10.0%		-6.1
2.5%		-6.1
0.5%		-6.1
0.0%	minimum	-6.1


Summary Statistics

Mean	-2.725
Std Dev	3.8395963
Std Err Mean	1.9197982
Upper 95% Mean	3.3846546
Lower 95% Mean	-8.834655
N	4

GrF Distribution by Detection Method

Distributions Analyte_Detection=Gross beta Gross
Alpha/Beta - 2 pi gas flow proportional counter

Bias

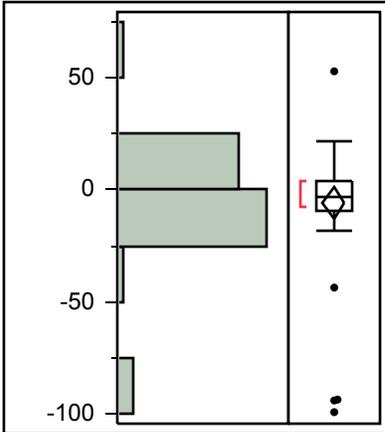

Quantiles

100.0%	maximum	52.8
99.5%		52.8
97.5%		41.1375
90.0%		15.55
75.0%	quartile	3.875
50.0%	median	-2.8
25.0%	quartile	-9.4
10.0%		-17.25
2.5%		-97.15
0.5%		-99.1
0.0%	minimum	-99.1


Summary Statistics

Mean	-5.605556
Std Dev	25.674239
Std Err Mean	3.4938215
Upper 95% Mean	1.4021628
Lower 95% Mean	-12.61327
N	54

GrF Distribution by Detection Method

Distributions
Analyte_Detection=Gross beta Other

Bias

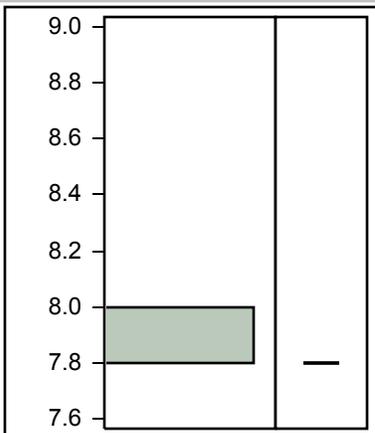

Quantiles

100.0%	maximum	7.8
99.5%		7.8
97.5%		7.8
90.0%		7.8
75.0%	quartile	7.8
50.0%	median	7.8
25.0%	quartile	7.8
10.0%		7.8
2.5%		7.8
0.5%		7.8
0.0%	minimum	7.8


Summary Statistics

Mean	7.8
Std Dev	.
Std Err Mean	.
Upper 95% Mean	.
Lower 95% Mean	.
N	1

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross alpha Acid
dissolution by strong Aqua Regia, hydrofluoric acid, etc.

Bias

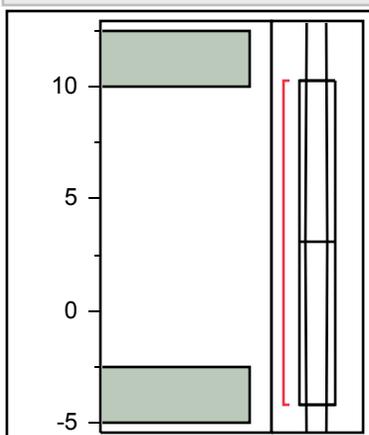

Quantiles

100.0%	maximum	10.3
99.5%		10.3
97.5%		10.3
90.0%		10.3
75.0%	quartile	10.3
50.0%	median	3.05
25.0%	quartile	-4.2
10.0%		-4.2
2.5%		-4.2
0.5%		-4.2
0.0%	minimum	-4.2


Summary Statistics

Mean	3.05
Std Dev	10.253048
Std Err Mean	7.25
Upper 95% Mean	95.169984
Lower 95% Mean	-89.06998
N	2

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross alpha
Acid leaching without hydrofluoric acid

Bias

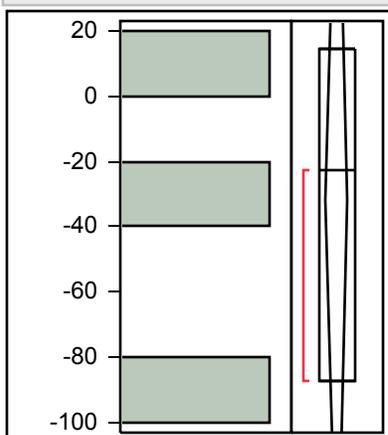

Quantiles

100.0%	maximum	14.2
99.5%		14.2
97.5%		14.2
90.0%		14.2
75.0%	quartile	14.2
50.0%	median	-22.6
25.0%	quartile	-87
10.0%		-87
2.5%		-87
0.5%		-87
0.0%	minimum	-87


Summary Statistics

Mean	-31.8
Std Dev	51.223432
Std Err Mean	29.573862
Upper 95% Mean	95.446059
Lower 95% Mean	-159.0461
N	3

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross alpha EPA 900,
Radioactivity, Gross Alpha/Beta Screening, 600/4-80-032

Bias

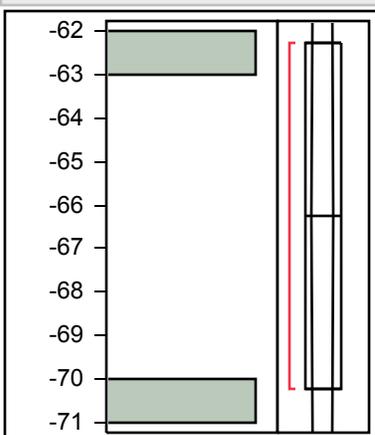

Quantiles

100.0%	maximum	-62.3
99.5%		-62.3
97.5%		-62.3
90.0%		-62.3
75.0%	quartile	-62.3
50.0%	median	-66.25
25.0%	quartile	-70.2
10.0%		-70.2
2.5%		-70.2
0.5%		-70.2
0.0%	minimum	-70.2


Summary Statistics

Mean	-66.25
Std Dev	5.5861436
Std Err Mean	3.95
Upper 95% Mean	-16.06049
Lower 95% Mean	-116.4395
N	2

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross
alpha Evaporation, acidified

Bias

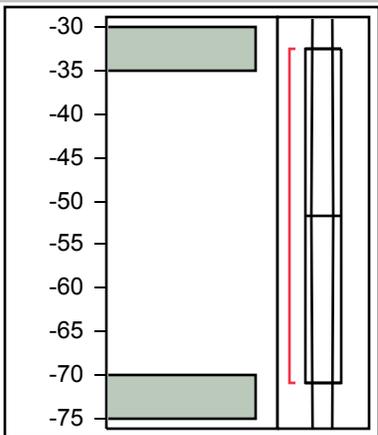

Quantiles

100.0%	maximum	-32.5
99.5%		-32.5
97.5%		-32.5
90.0%		-32.5
75.0%	quartile	-32.5
50.0%	median	-51.65
25.0%	quartile	-70.8
10.0%		-70.8
2.5%		-70.8
0.5%		-70.8
0.0%	minimum	-70.8


Summary Statistics

Mean	-51.65
Std Dev	27.08219
Std Err Mean	19.15
Upper 95% Mean	191.67382
Lower 95% Mean	-294.9738
N	2

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross alpha
No preparation - analyzed as received

Bias

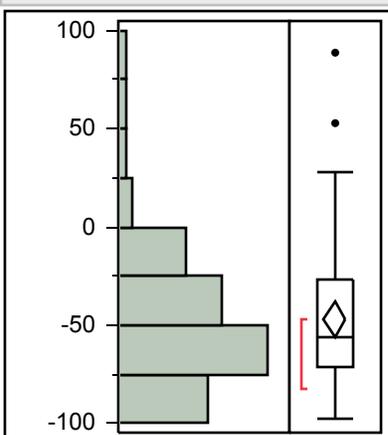

Quantiles

100.0%	maximum	88.7
99.5%		88.7
97.5%		69.8525
90.0%		-7.52
75.0%	quartile	-26.9
50.0%	median	-55.95
25.0%	quartile	-71.55
10.0%		-79.81
2.5%		-94.675
0.5%		-97.3
0.0%	minimum	-97.3

Summary Statistics


Mean	-46.75
Std Dev	35.258034
Std Err Mean	4.5517927
Upper 95% Mean	-37.64188
Lower 95% Mean	-55.85812
N	60

GrF Distribution by Prep Method

Distributions

Analyte_Method=Gross alpha Other

Bias

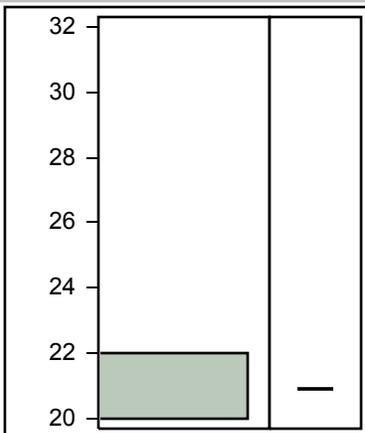

Quantiles

100.0%	maximum	20.9
99.5%		20.9
97.5%		20.9
90.0%		20.9
75.0%	quartile	20.9
50.0%	median	20.9
25.0%	quartile	20.9
10.0%		20.9
2.5%		20.9
0.5%		20.9
0.0%	minimum	20.9


Summary Statistics

Mean	20.9
Std Dev	.
Std Err Mean	.
Upper 95% Mean	.
Lower 95% Mean	.
N	1

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross alpha Wet ash -
Acid digestion - the use of oxidizers to destroy organics

Bias

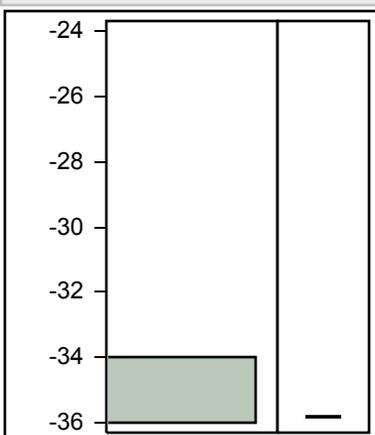

Quantiles

100.0%	maximum	-35.8
99.5%		-35.8
97.5%		-35.8
90.0%		-35.8
75.0%	quartile	-35.8
50.0%	median	-35.8
25.0%	quartile	-35.8
10.0%		-35.8
2.5%		-35.8
0.5%		-35.8
0.0%	minimum	-35.8


Summary Statistics

Mean	-35.8
Std Dev	.
Std Err Mean	.
Upper 95% Mean	.
Lower 95% Mean	.
N	1

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross beta Acid
dissolution by strong Aqua Reqia, hydrofluoric acid, etc.

Bias

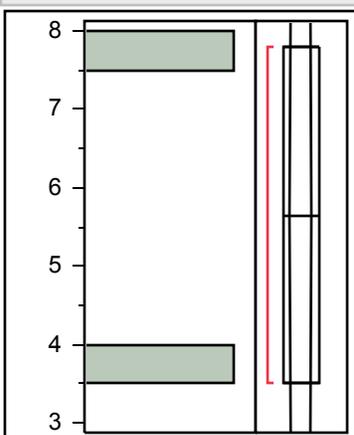

Quantiles

100.0%	maximum	7.8
99.5%		7.8
97.5%		7.8
90.0%		7.8
75.0%	quartile	7.8
50.0%	median	5.65
25.0%	quartile	3.5
10.0%		3.5
2.5%		3.5
0.5%		3.5
0.0%	minimum	3.5


Summary Statistics

Mean	5.65
Std Dev	3.0405592
Std Err Mean	2.15
Upper 95% Mean	32.96834
Lower 95% Mean	-21.66834
N	2

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross beta
Acid leaching without hydrofluoric acid

Bias

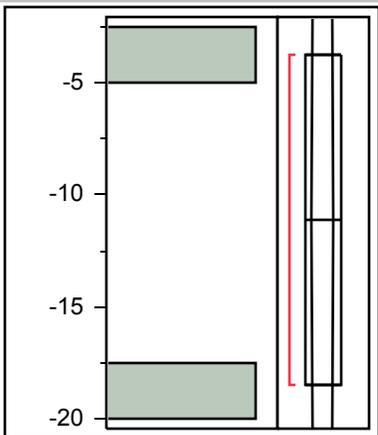

Quantiles

100.0%	maximum	-3.8
99.5%		-3.8
97.5%		-3.8
90.0%		-3.8
75.0%	quartile	-3.8
50.0%	median	-11.15
25.0%	quartile	-18.5
10.0%		-18.5
2.5%		-18.5
0.5%		-18.5
0.0%	minimum	-18.5


Summary Statistics

Mean	-11.15
Std Dev	10.39447
Std Err Mean	7.35
Upper 95% Mean	82.240605
Lower 95% Mean	-104.5406
N	2

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross beta EPA 900,
Radioactivity, Gross Alpha/Beta Screening, 600/4-80-032

Bias

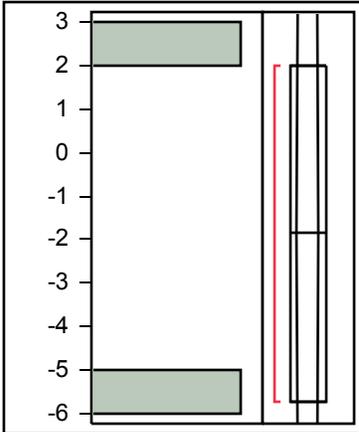

Quantiles

100.0%	maximum	2
99.5%		2
97.5%		2
90.0%		2
75.0%	quartile	2
50.0%	median	-1.85
25.0%	quartile	-5.7
10.0%		-5.7
2.5%		-5.7
0.5%		-5.7
0.0%	minimum	-5.7


Summary Statistics

Mean	-1.85
Std Dev	5.4447222
Std Err Mean	3.85
Upper 95% Mean	47.068888
Lower 95% Mean	-50.76889
N	2

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross
beta Evaporation, acidified

Bias

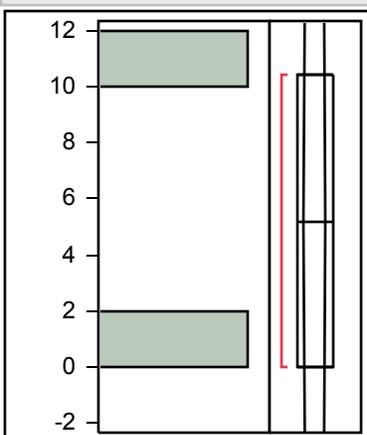

Quantiles

100.0%	maximum	10.4
99.5%		10.4
97.5%		10.4
90.0%		10.4
75.0%	quartile	10.4
50.0%	median	5.2
25.0%	quartile	0
10.0%		0
2.5%		0
0.5%		0
0.0%	minimum	0


Summary Statistics

Mean	5.2
Std Dev	7.3539105
Std Err Mean	5.2
Upper 95% Mean	71.272265
Lower 95% Mean	-60.87226
N	2

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross beta
No preparation - analyzed as received

Bias

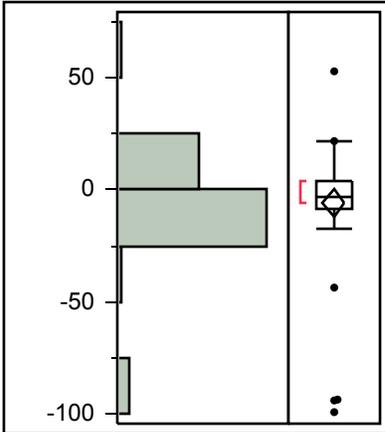

Quantiles

100.0%	maximum	52.8
99.5%		52.8
97.5%		35.695
90.0%		14.98
75.0%	quartile	3.5
50.0%	median	-2.8
25.0%	quartile	-8.6
10.0%		-16
2.5%		-96.24
0.5%		-99.1
0.0%	minimum	-99.1

Summary Statistics


Mean	-5.659016
Std Dev	24.162405
Std Err Mean	3.0936789
Upper 95% Mean	0.5292627
Lower 95% Mean	-11.8473
N	61

GrF Distribution by Prep Method

Distributions

Analyte_Method=Gross beta Other

Bias

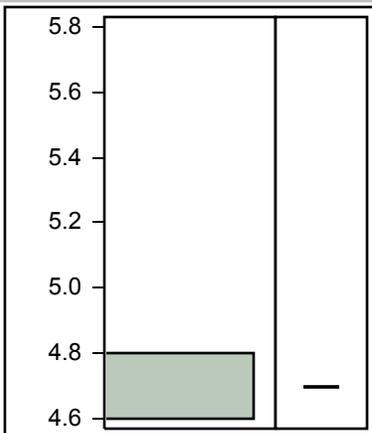

Quantiles

100.0%	maximum	4.7
99.5%		4.7
97.5%		4.7
90.0%		4.7
75.0%	quartile	4.7
50.0%	median	4.7
25.0%	quartile	4.7
10.0%		4.7
2.5%		4.7
0.5%		4.7
0.0%	minimum	4.7


Summary Statistics

Mean	4.7
Std Dev	.
Std Err Mean	.
Upper 95% Mean	.
Lower 95% Mean	.
N	1

GrF Distribution by Prep Method

Distributions Analyte_Method=Gross beta Wet ash - Acid digestion - the use of oxidizers to destroy organics

Bias

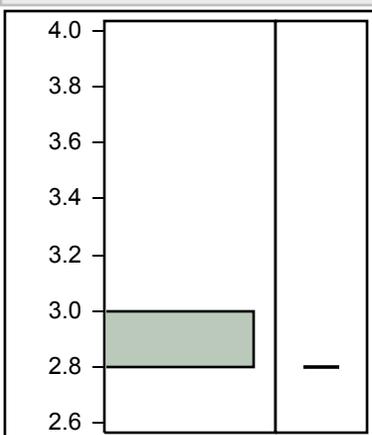

Quantiles

100.0%	maximum	2.8
99.5%		2.8
97.5%		2.8
90.0%		2.8
75.0%	quartile	2.8
50.0%	median	2.8
25.0%	quartile	2.8
10.0%		2.8
2.5%		2.8
0.5%		2.8
0.0%	minimum	2.8

Summary Statistics

Mean	2.8
Std Dev	.
Std Err Mean	.
Upper 95% Mean	.
Lower 95% Mean	.
N	1